


Aka-Brief #1 Brass

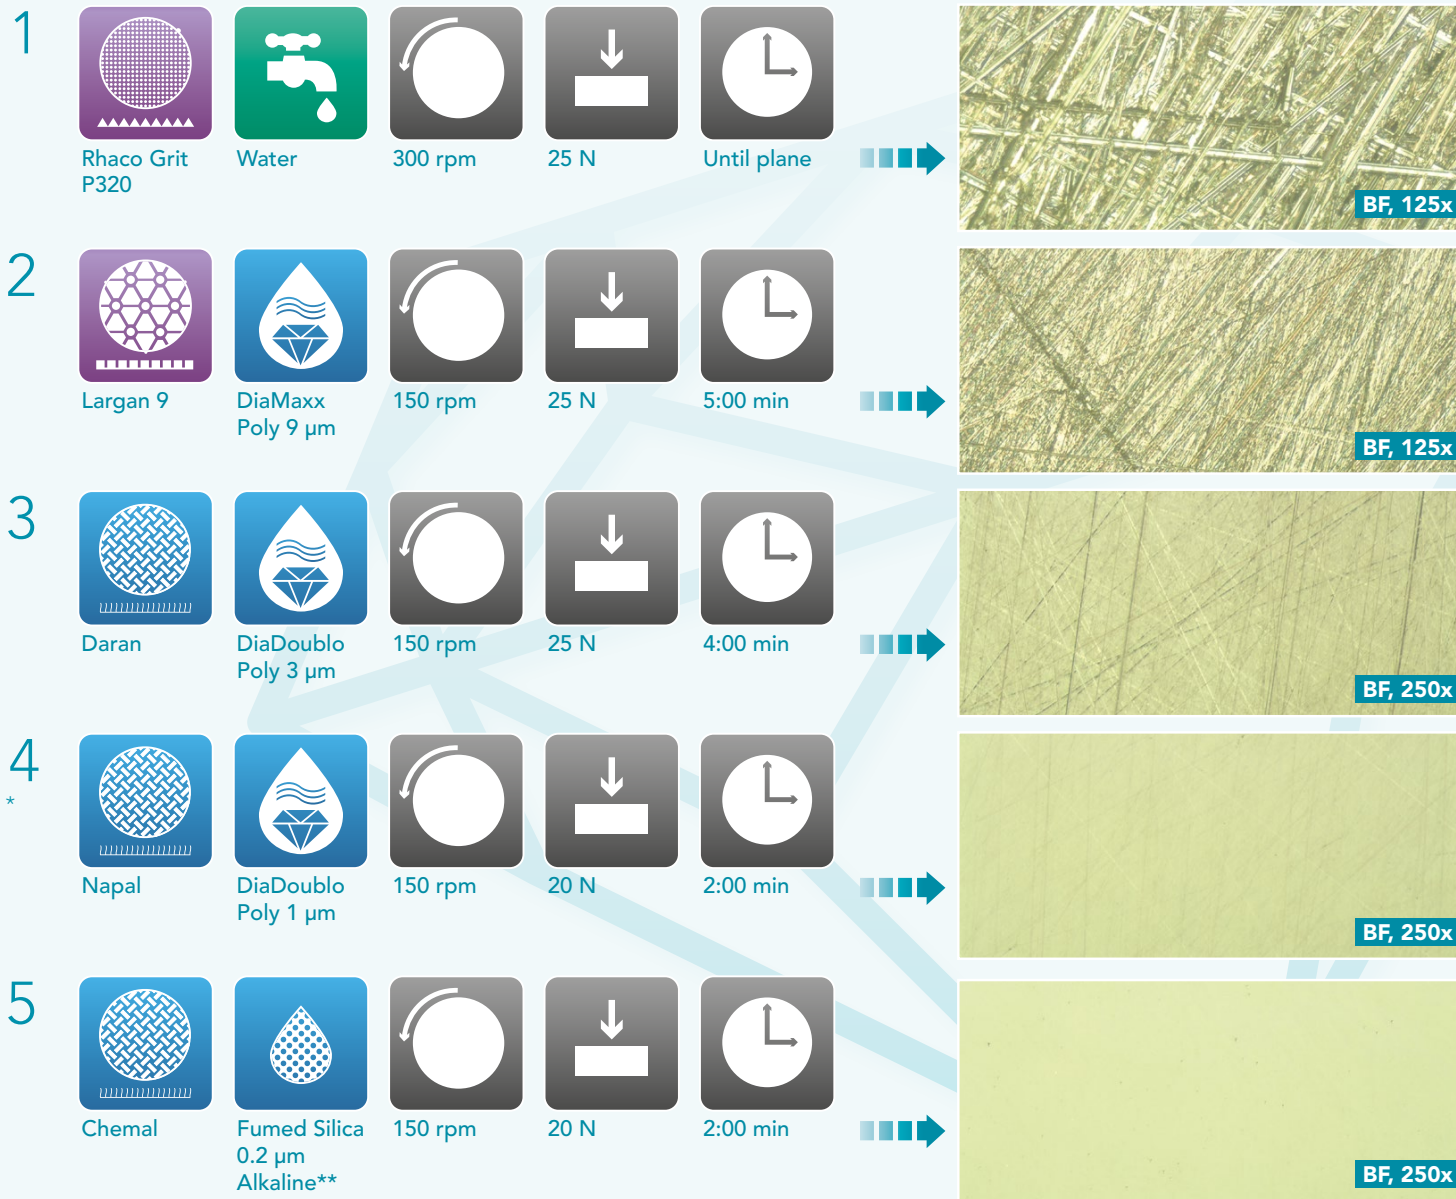

Times are stated for a 300 mm preparation system and 40 mm dia. samples.
On a 250 mm system the times should be increased by 30%, on a 200 mm system by 100%.
With larger samples the force should be increased, with smaller samples decreased.

Time and Force may vary depending on the equipment.

* Step 4 is optional

** 96 ml Fumed Silica,
2 ml H₂O₂ (30%),
2 ml NH₄OH (25%).